


Instructions for Use

REF DIATUBE002

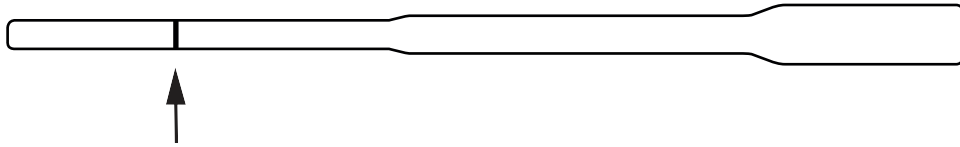


Fill line indicates target volume

Step 1

Hold tube horizontally, touch tip to blood collection site.

Gently squeeze bulb to draw blood into the tube.

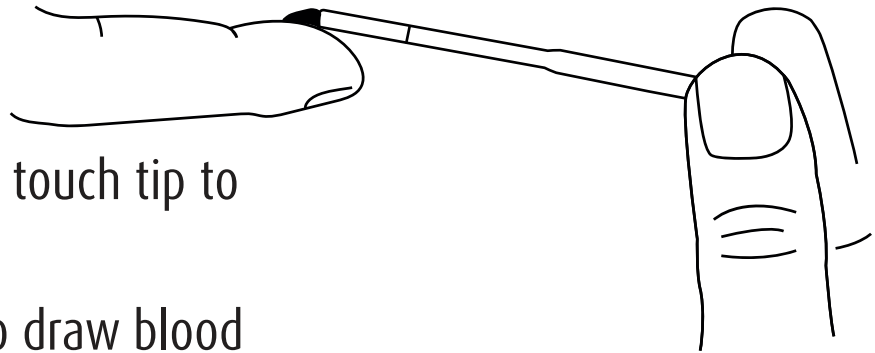

Step 2

Expel sample by aligning the tip of the tube with the testing site or vial and squeezing bulb.

If sample was not collected to fill line it may not expel. Repeat Step 1 and proceed to Step 2.

